


S1: (arrow mark) HRs > 99.9 + HRp > 99.8% @ 515 nm, AOI 45 deg  
S2: ARp < 0.1% @ 515 nm, AOI 45 deg.

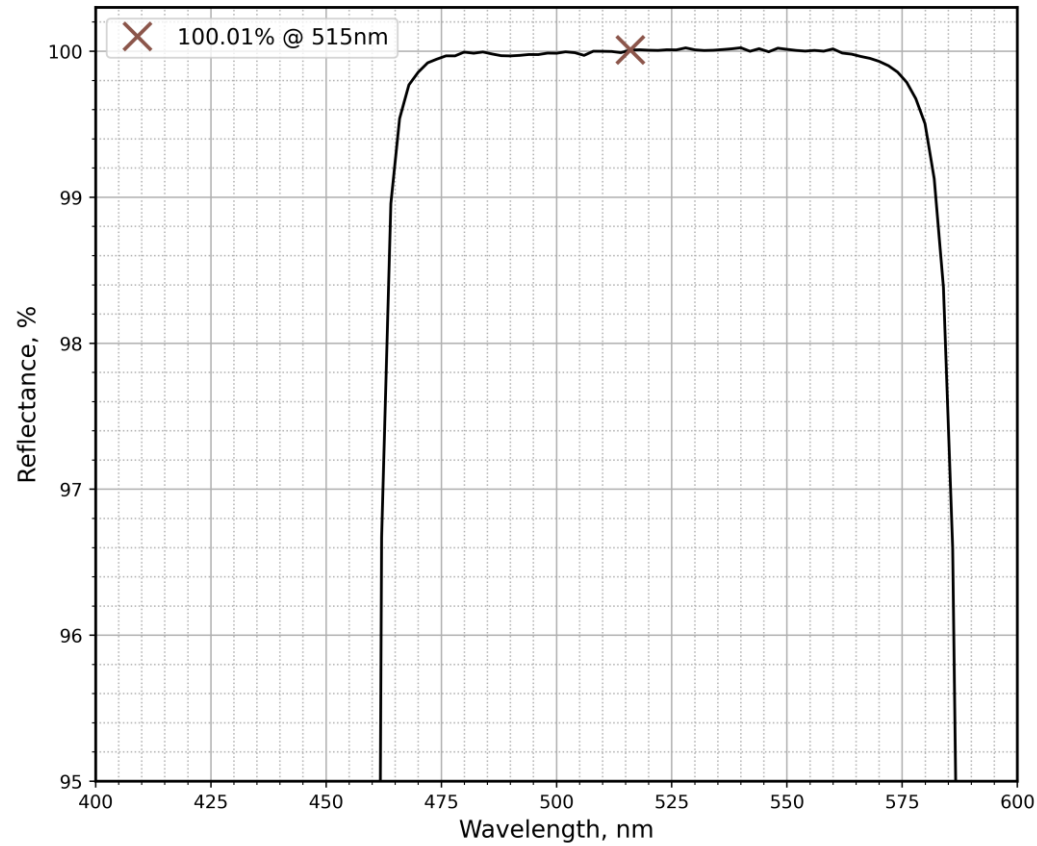


PO2785 Rs i45

Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%

S1: (arrow mark) HRs > 99.9 + HRp > 99.8% @ 515 nm, AOI 45 deg  
S2: ARp < 0.1% @ 515 nm, AOI 45 deg.

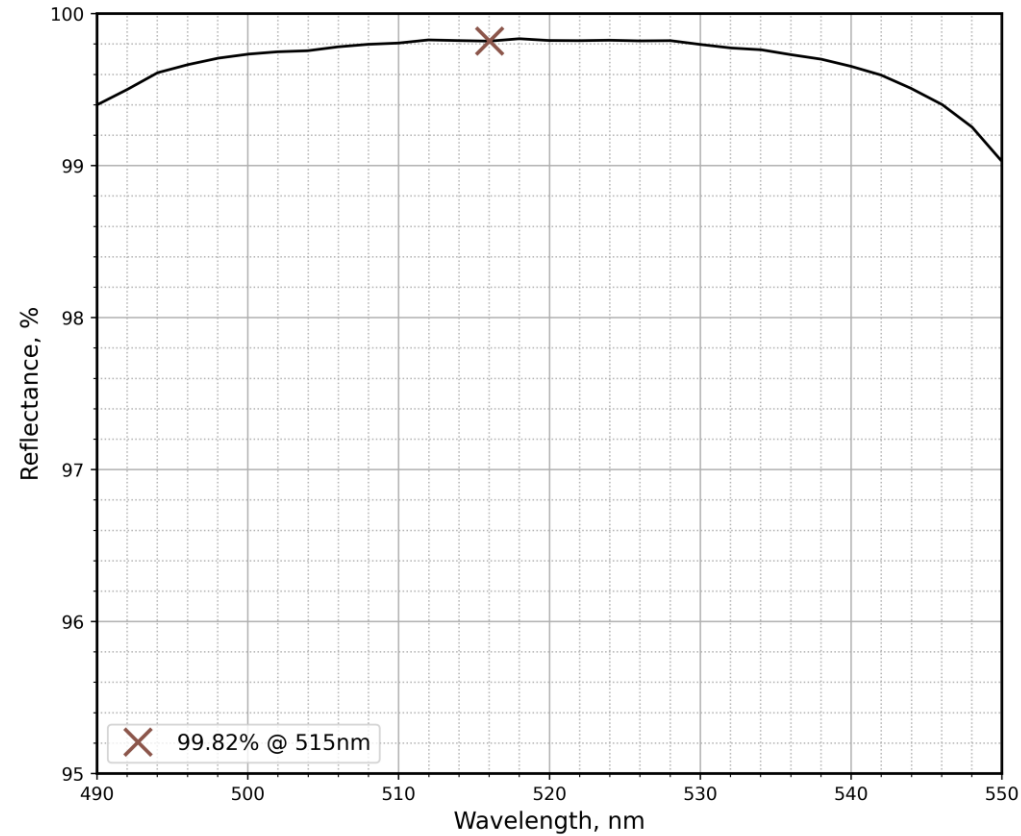

PO2785 Rp i45

Fig. 2.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%