

S1: HRsp > 99.8% @ 1030 nm + 515 nm |GDDr ~ 0 fss| @ 1030 nm + 515 nm, AOI 45 deg
S2: uncoated

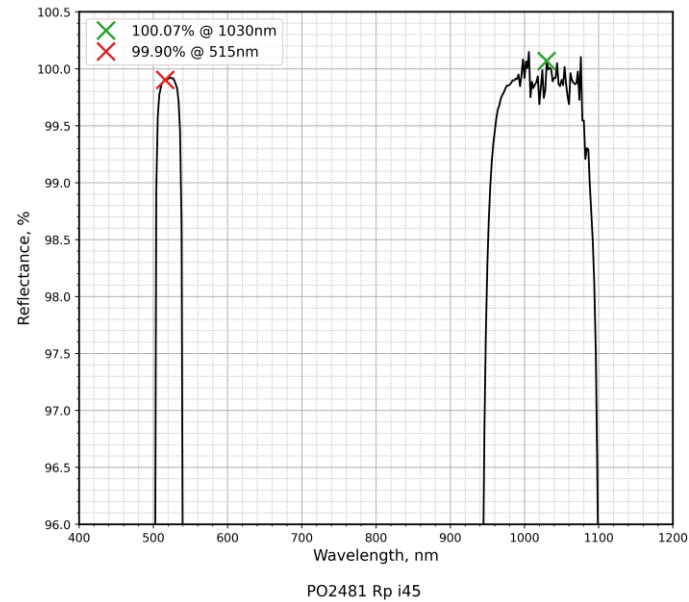


Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%

S1: HRsp > 99.8% @ 1030 nm + 515 nm |GDDr ~ 0 fss| @ 1030 nm + 515 nm, AOI 45 deg
S2: uncoated

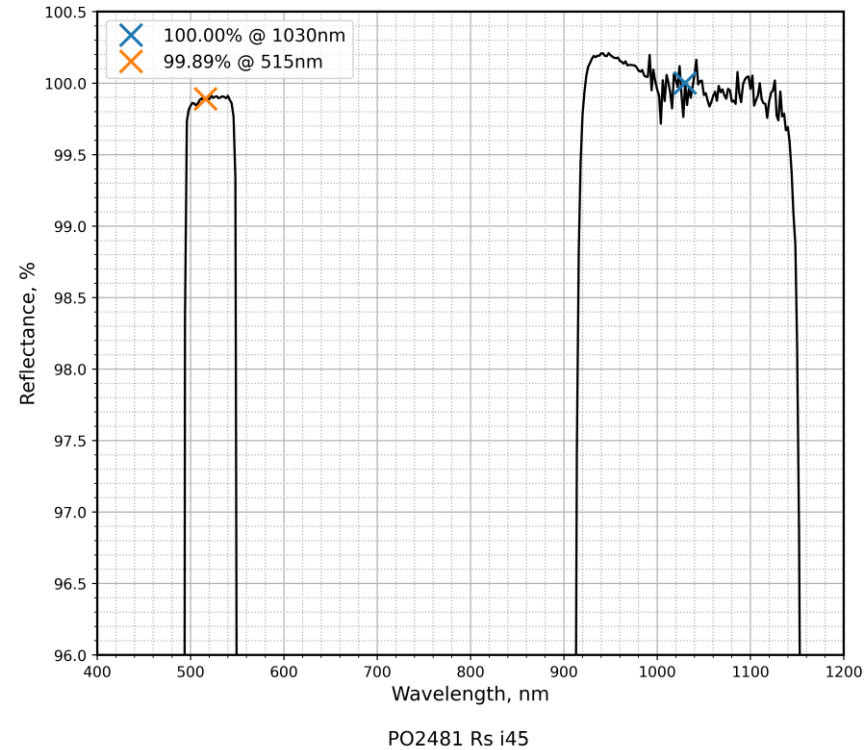


Fig. 2.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%