

S1: (arrow marks) HRs > 99.9% @ 385-415 nm + 770-830 nm HRp > 99.8% @ 395-415 nm + HRp > 99.9% @ 770-820 nm
 S2: uncoated

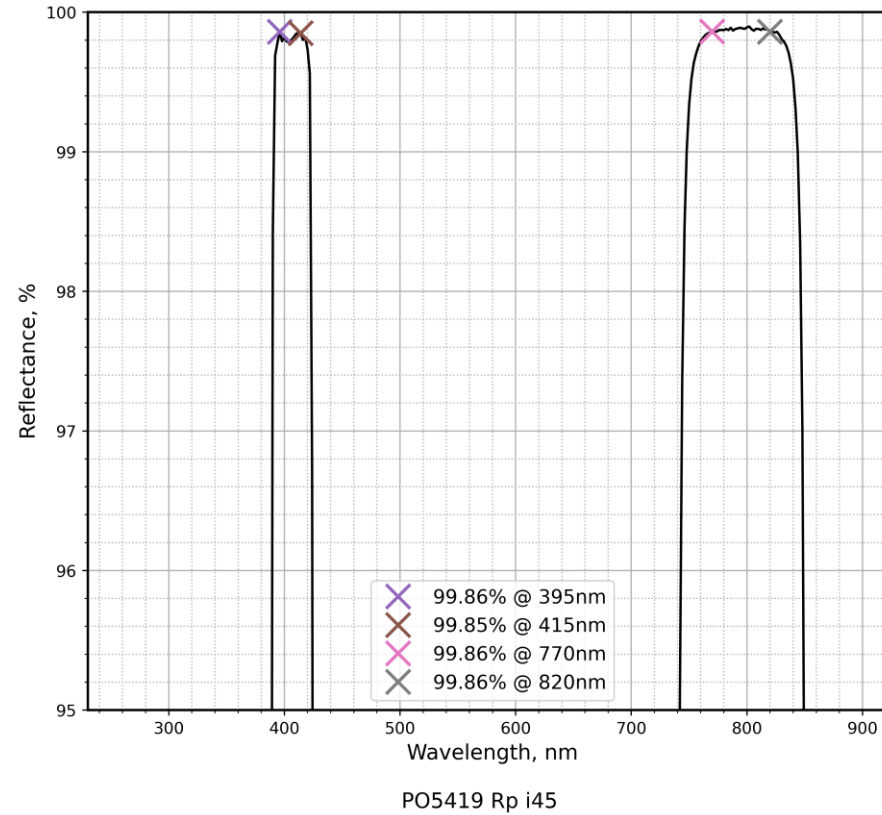


Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%

S1: (arrow marks) HRs > 99.9% @ 385-415 nm + 770-830 nm HRp > 99.8% @ 395-415 nm + HRp > 99.9% @ 770-820 nm
 S2: uncoated

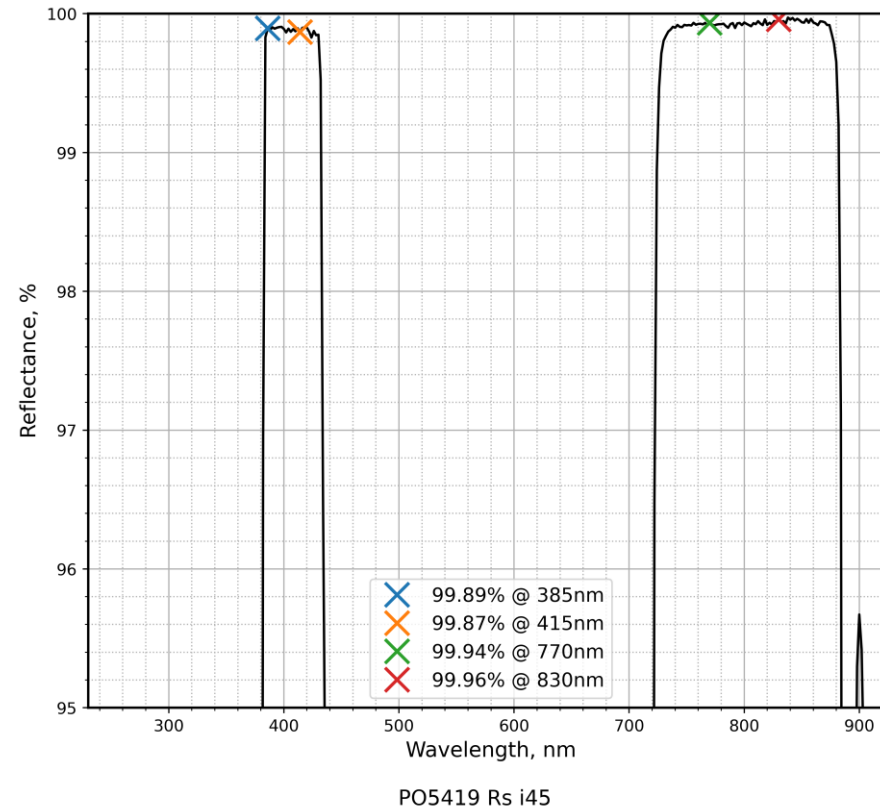


Fig. 2.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%