


S1:HRa>99.3%@343 nm + HRa>99.5%@515 nm + HRa>99.8%@1030 nm, AOI = 45 deg; GDD_Rsp <+/-50fs²@ 343, 515, 1030 nm, AOI = 45 deg
S2:SCC

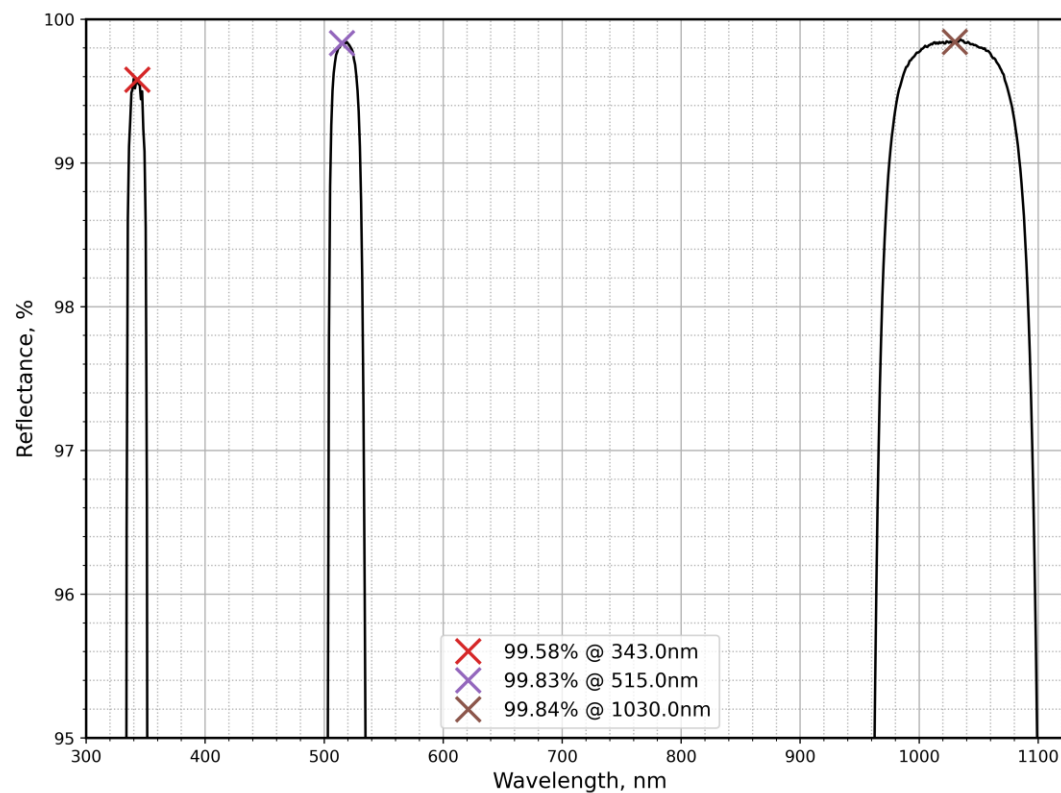

PO13596 Ra i45

Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.1%