

S1: (arrow marks) PRs=96.8% +/-0.2% @ 1150 nm, AOI 45 deg.
S2: ARs<0.1% @ 1150 nm, 45 deg.

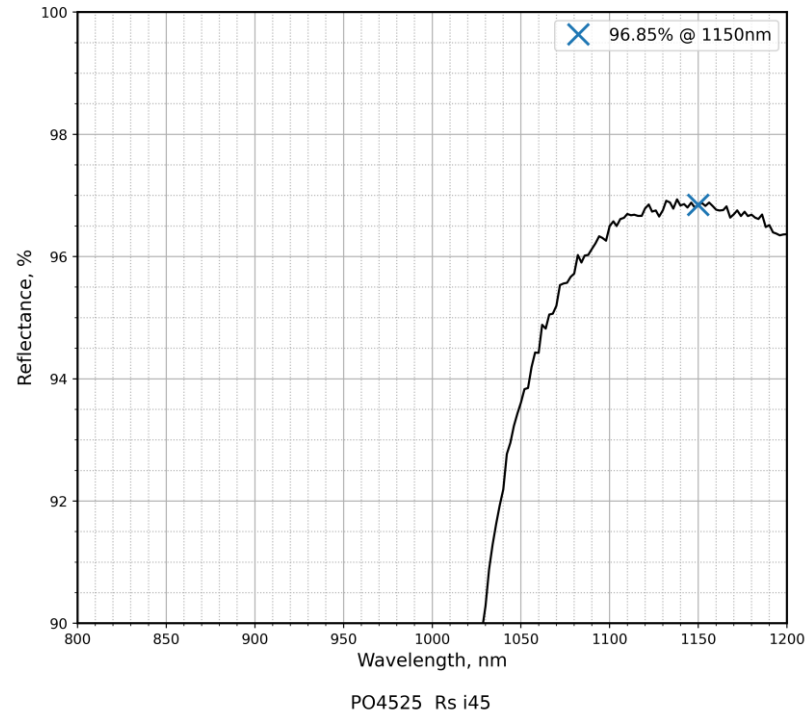


Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%

S1: (arrow marks) PRs=96.8% +/-0.2% @ 1150 nm, AOI 45 deg.
S2: ARs<0.1% @ 1150 nm, 45 deg.

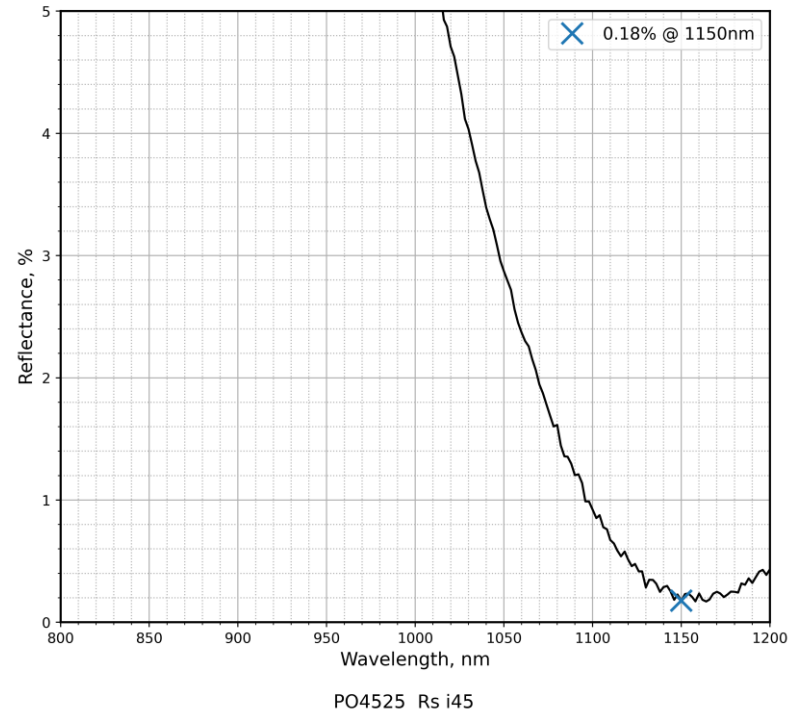


Fig. 2.

SIDE MEASURED: S2 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%