


S1: (arrow marks) PRs = 95% +/-2% @ 1064 nm + 532 nm, AOI 45 deg
S2: uncoated

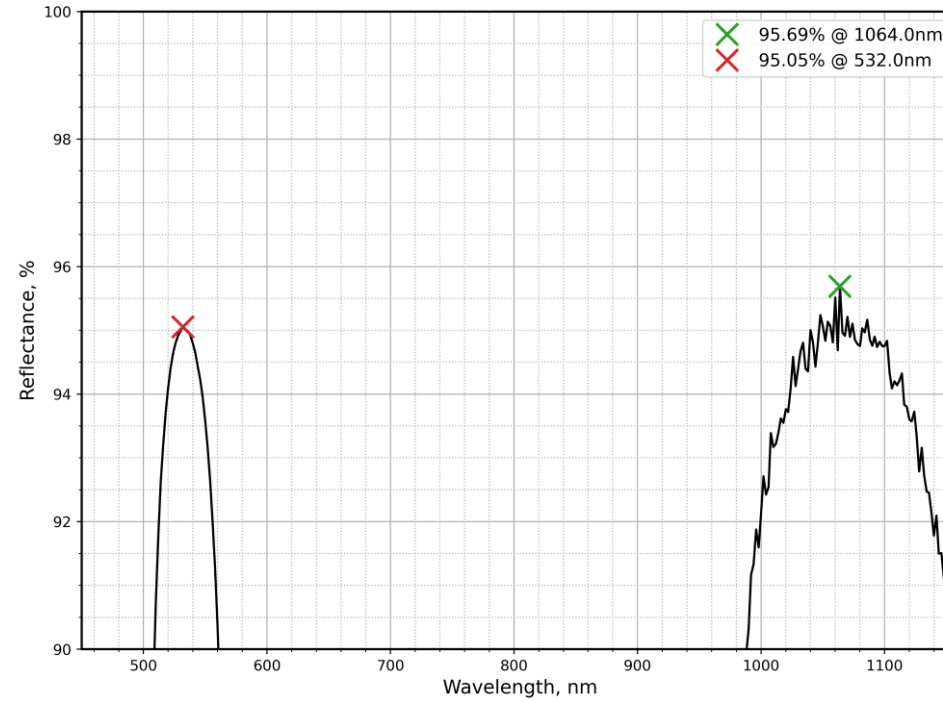

PO7732 Rs i45

Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%