


S1:(arrow marks) PRs = 99.5% +/-0.2% @ 1020-1040 nm, AOI=45 deg  
S2: ARs<0.1% @ 1020-1040 nm, AOI 45 deg

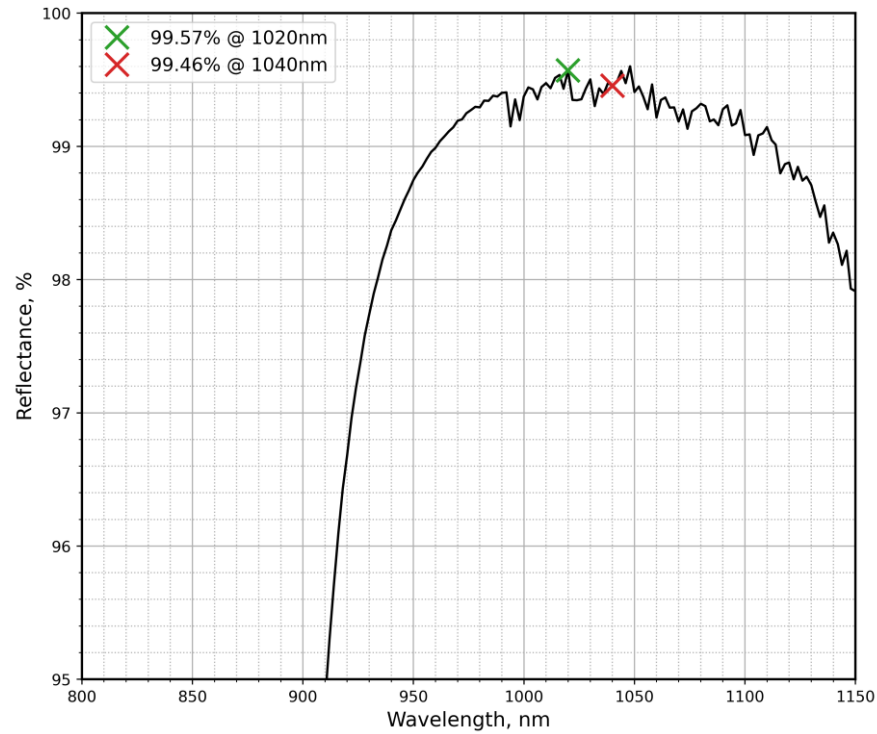

PO4276 Rs i45

Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%