

S1: HRp>99.5%@ 327-363nm, HRs>99.75%@320 - 370 nm AOI=45 deg. GDD Rs=0 +/-10 fs² @ 320 - 370 nm / AOI=45 deg. GDD Rp=0 +/-10 fs² @ 330 - 360 nm / AOI=45 deg.
S2: Uncoated

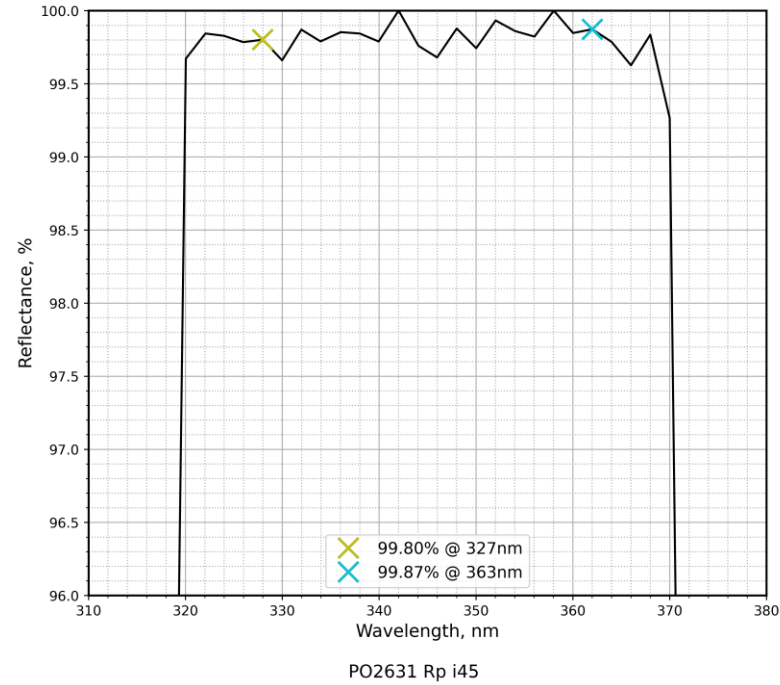


Fig. 1.

SIDE MEASURED: S1 only (witness sample)

COMMENTS: Margin of measurement error: +/-0.25%

S1: HRp>99.5%@ 327-363nm, HRs>99.75%@320 - 370 nm AOI=45 deg. GDD Rs=0 +/-10 fs² @ 320 - 370 nm / AOI=45 deg. GDD Rp=0 +/-10 fs² @ 330 - 360 nm / AOI=45 deg.
S2: Uncoated

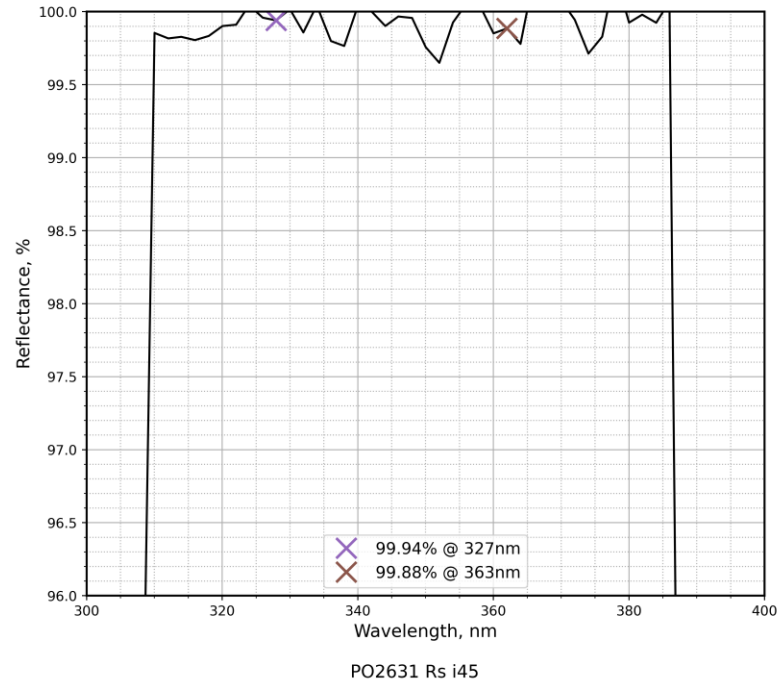


Fig. 2.

SIDE MEASURED: S1 only (witness sample)

COMMENTS: Margin of measurement error: +/-0.25%