

S1: (arrow marks) HRa>99.9% @ 1030 nm, AOI=0-45° |GDD R| <30 fs2 @ 1030 nm, AOI=0-45°
S2: Uncoated

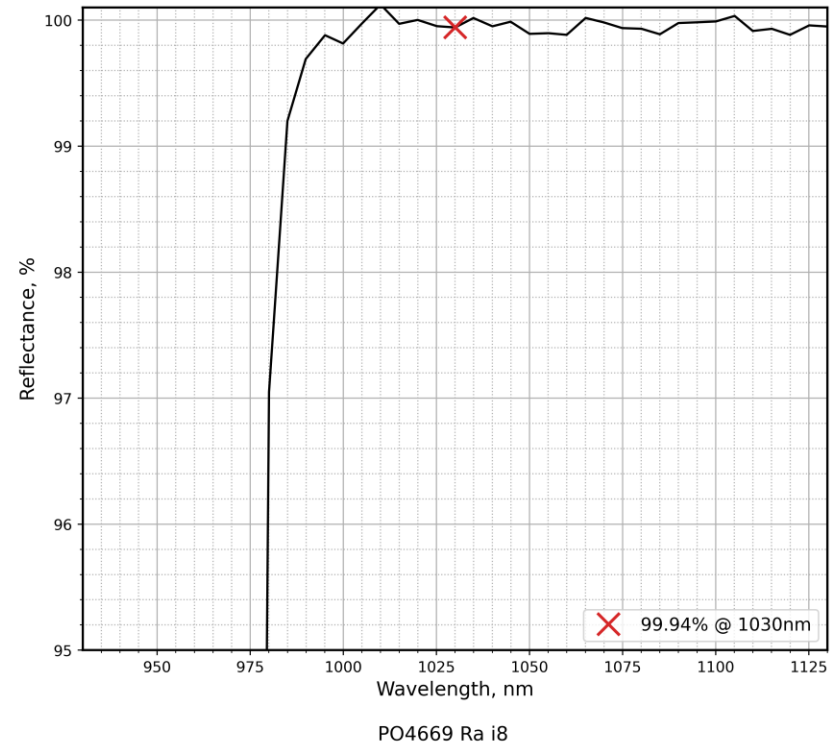


Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%

S1: (arrow marks) HRa>99.9% @ 1030 nm, AOI=0-45° |GDD R| <30 fs2 @ 1030 nm, AOI=0-45°
S2: Uncoated

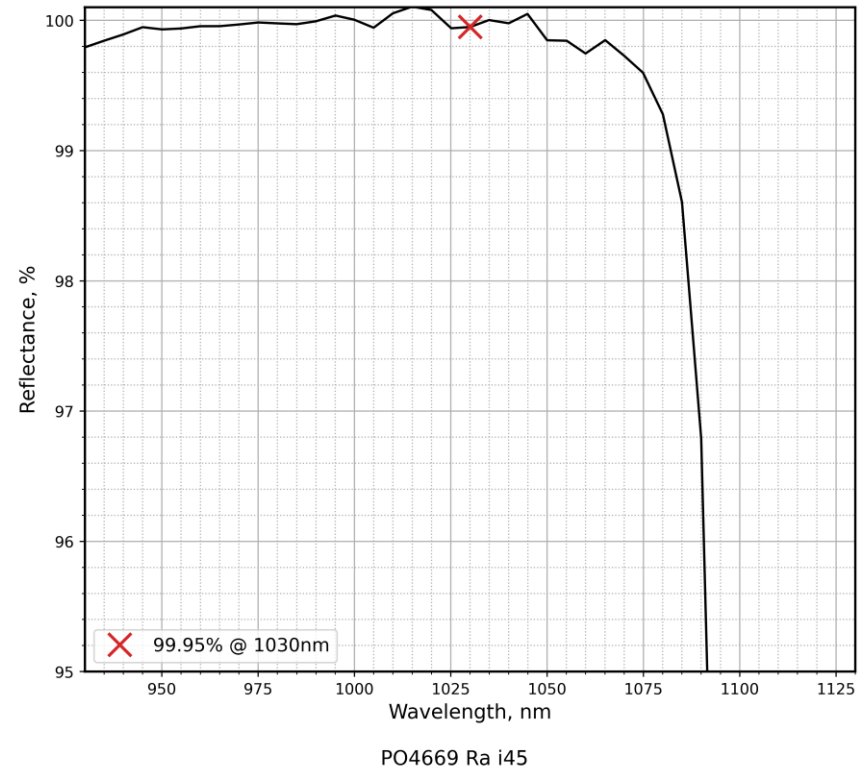


Fig. 2.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%