


S1 (arrow marks): HRs>99.95% & HRp>99.9%@1010 - 1050 nm, AOI=45°, |GDD Rs|<10 fs<sup>2</sup>, |GDD Rp|<20 fs<sup>2</sup>  
 S2: uncoated

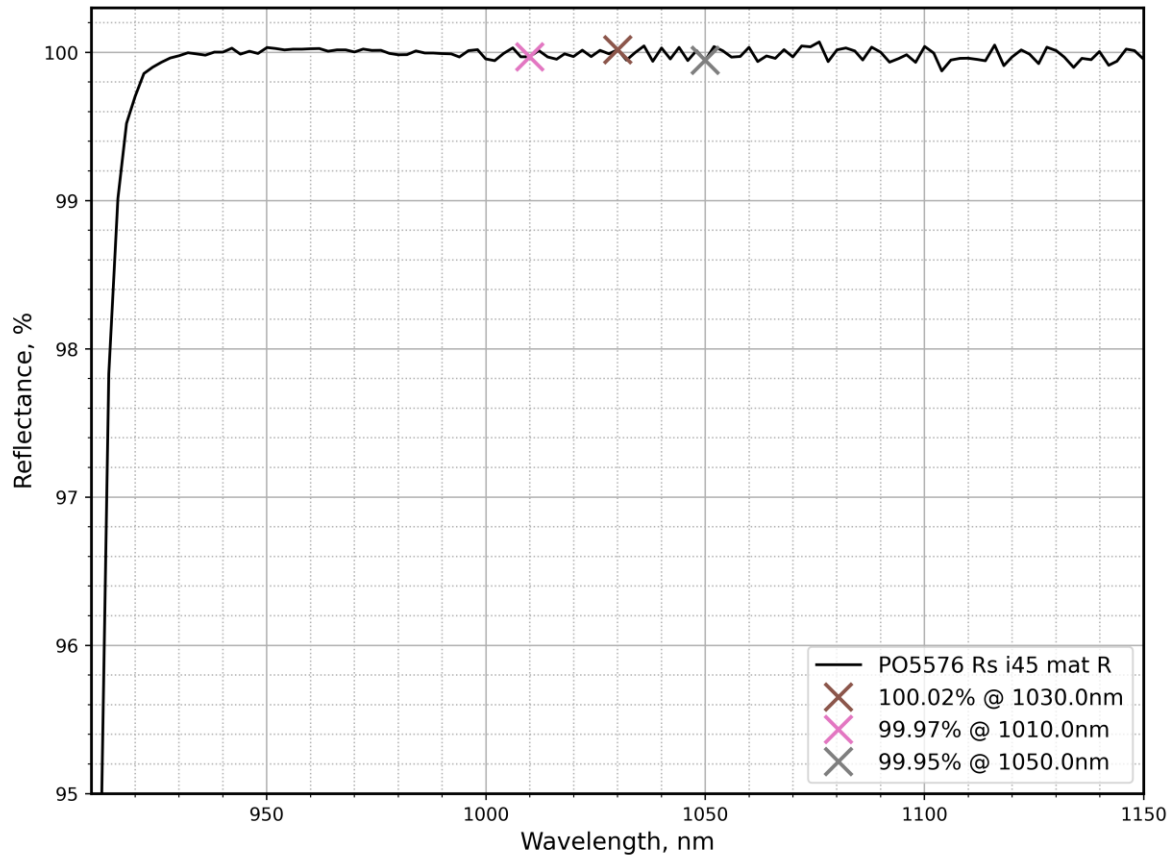

PO5576 Rs i45

Fig. 1.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/-0.25%

S1 (arrow marks): HRs > 99.95% & HRp > 99.9% @ 1010 - 1050 nm, AOI = 45°, |GDD Rs| < 10 fs<sup>2</sup>, |GDD Rp| < 20 fs<sup>2</sup>  
 S2: uncoated

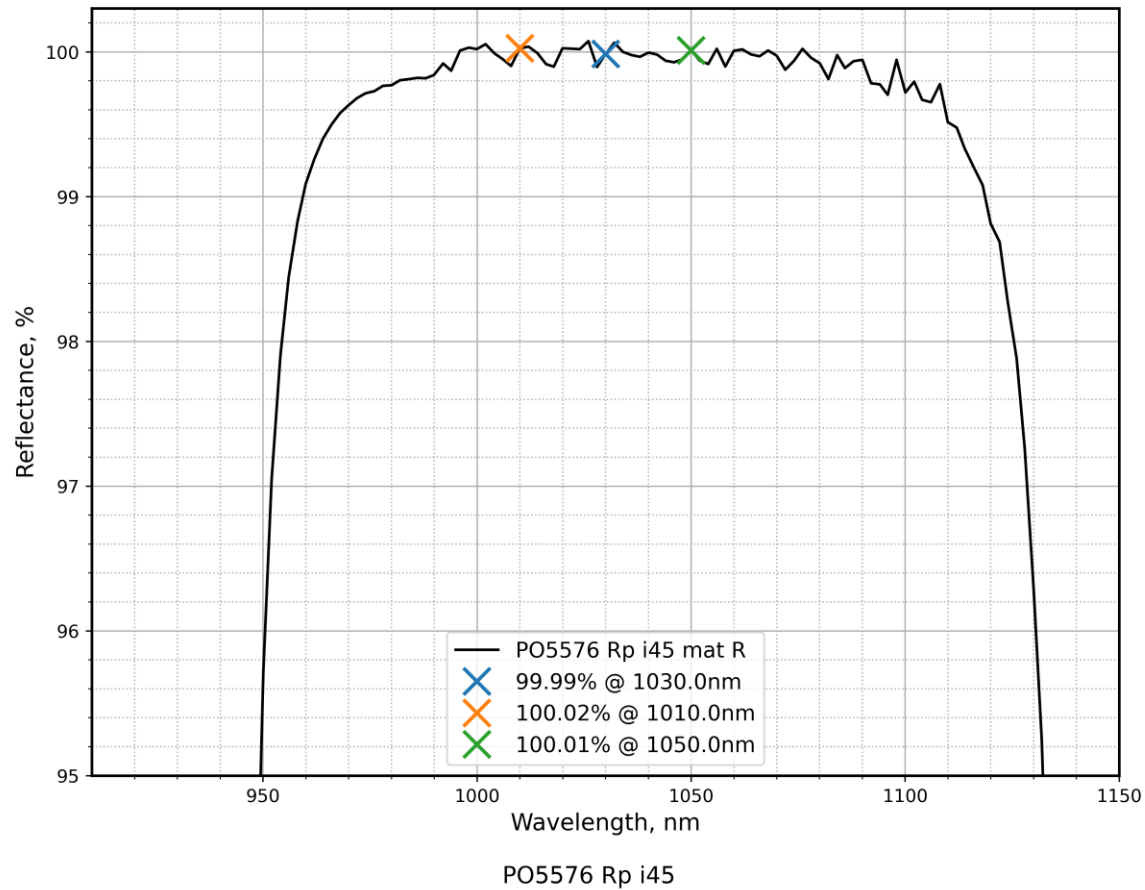


Fig. 2.

SIDE MEASURED: S1 only (grinded witness sample)

COMMENTS: Margin of measurement error: +/- 0.25%